


Unjointed Finger Probe -- UFP20

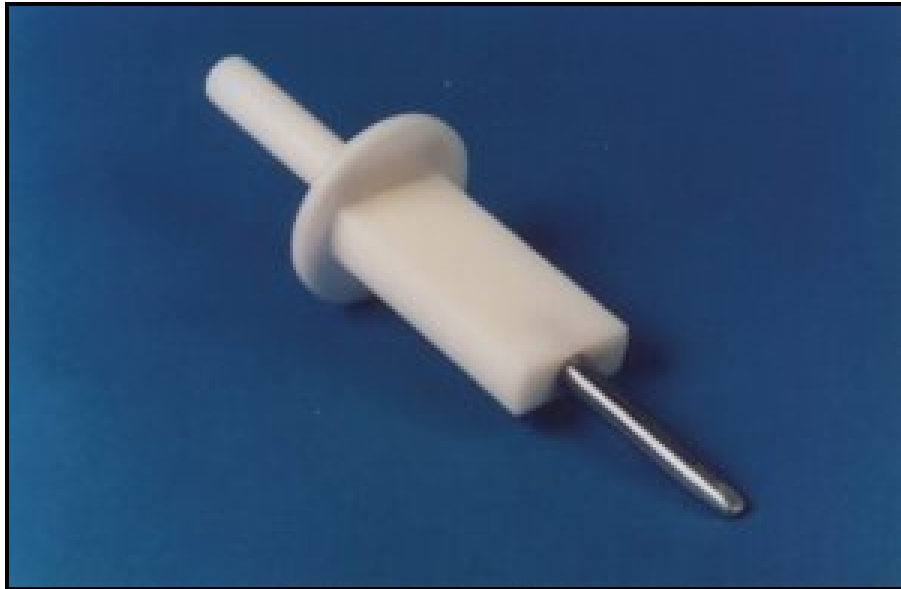

The Unjointed Finger Probe is made for forceful insertion where the flexibility of the Jointed Finger Probe would be a hindrance. The UFP20 meets IEC 60950 and 61010, CSA and UL requirements. This probe is made of stainless steel and the rest of the instrument of Delrin®. The handle is designed with a threaded hole for use with force gauges.